


Name: _____

Date: _____

STERILE PROCESSING

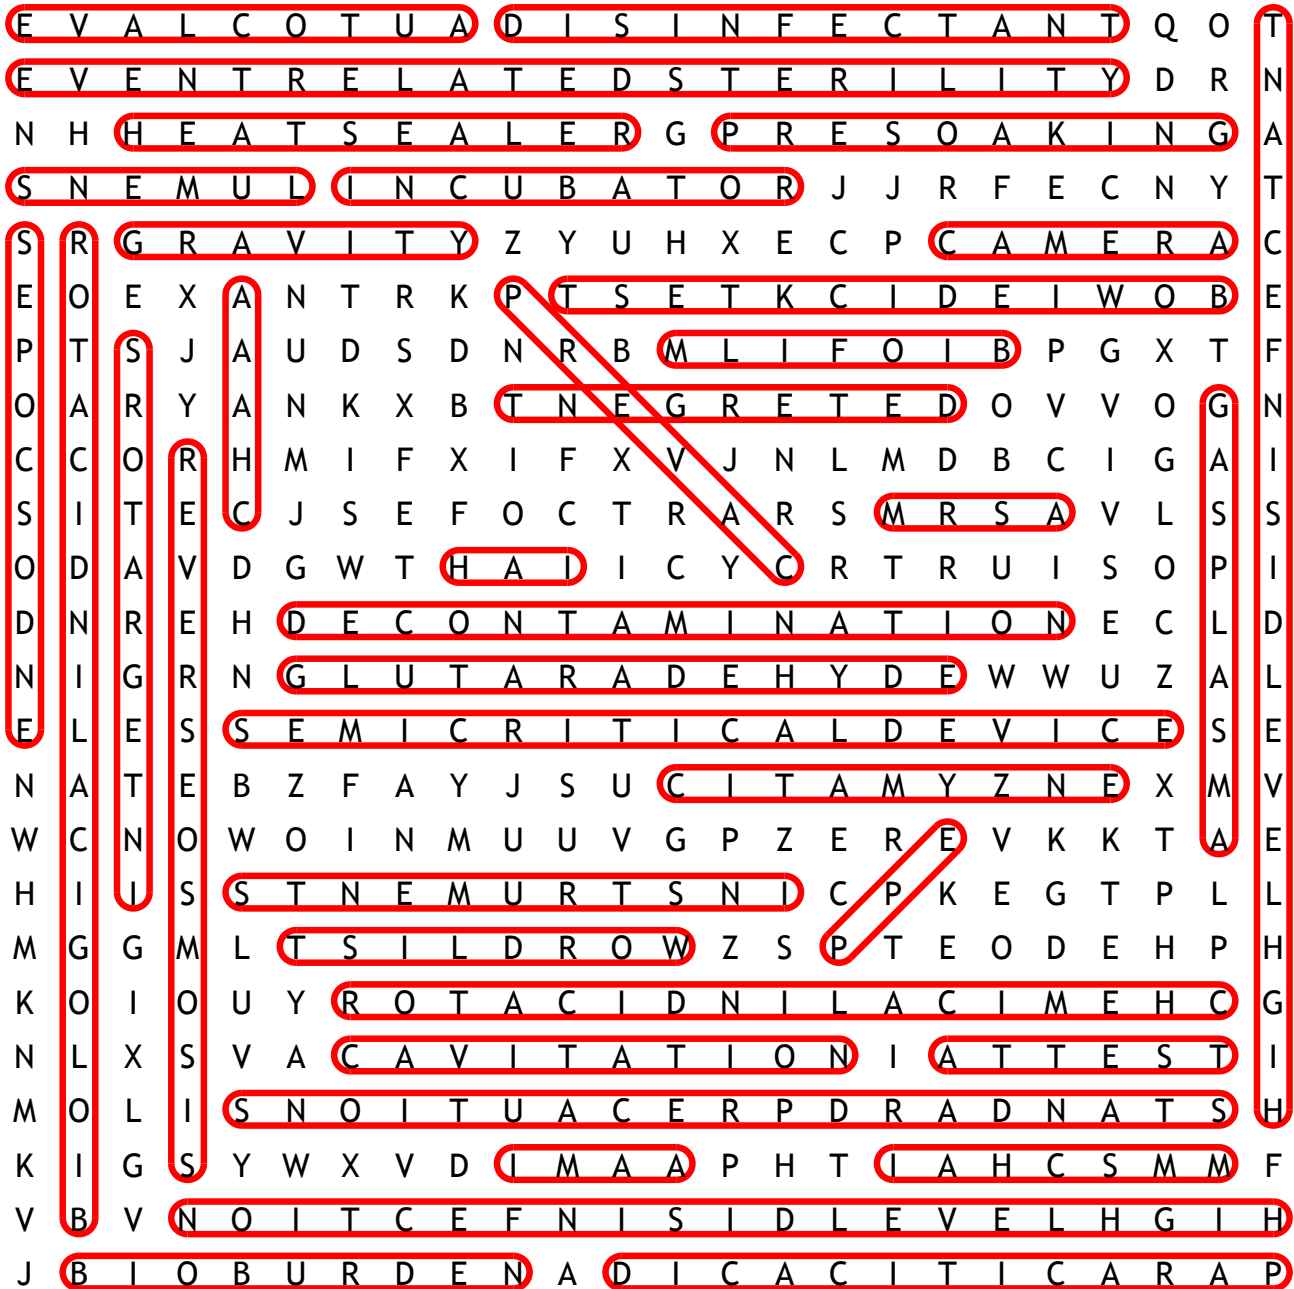

EVENT RELATED STERILITY
 SEMI CRITICAL DEVICE
 DECONTAMINATION
 DISINFECTANT
 CAVITATION
 WORD LIST:
 ENZYMATIC
 IAHCSMM
 PREVAC
 HAI

HIGH LEVEL DISINFECTANT
 STANDARD PRECAUTIONS
 REVERSE OSMOSIS
 HEAT SEALER
 ENDOSCOPES
 AUTOCLAVE
 INCUBATOR
 ATTEST
 AAAHC
 PPE

HIGH LEVEL DISINFECTION
 CHEMICAL INDICATOR
 PARACITIC ACID
 INSTRUMENTS
 GAS PLASMA
 BIOBURDEN
 BIOFILM
 CAMERA
 AAMI

BIOLOGICAL INDICATOR
 BOWIE DICK TEST
 GLUTARADEHYDE
 INTEGRATORS
 PRESOAKING
 DETERGENT
 GRAVITY
 LUMENS
 MRSA